

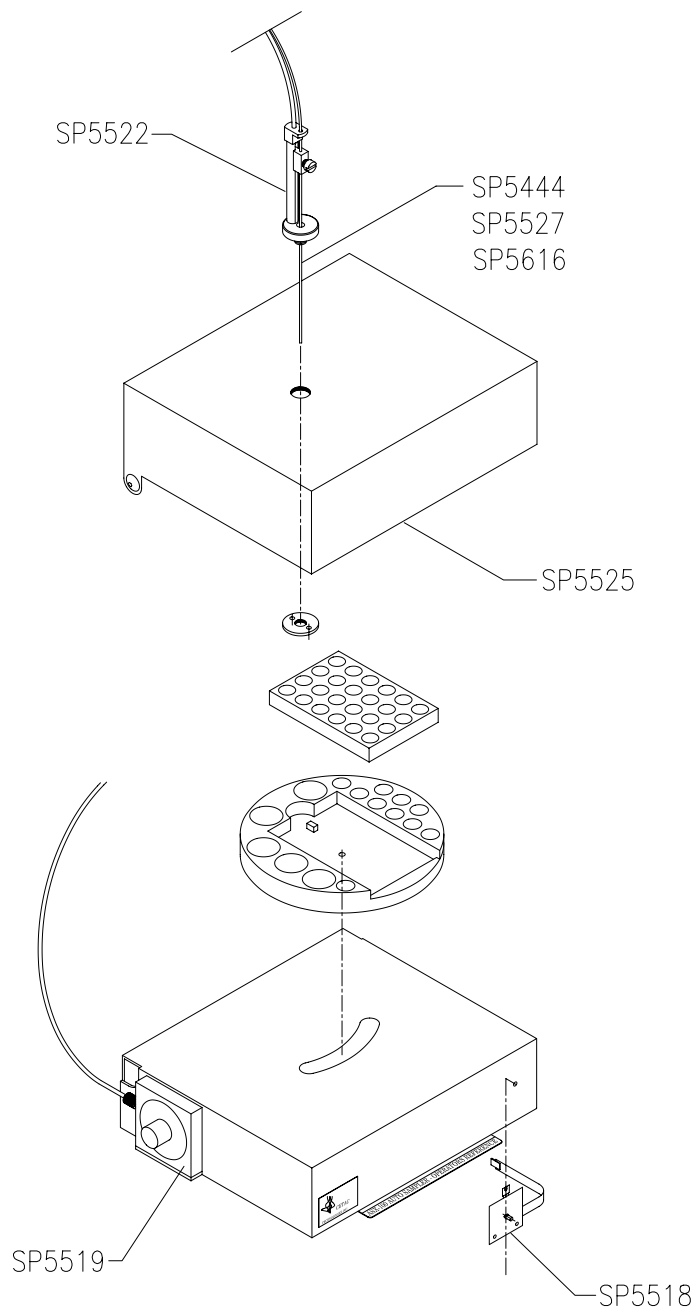
**ASX-100
RANDOM ACCESS MICRO AUTO SAMPLER
*OPERATOR'S ACCESSORIES AND
SUPPLIES CATALOG***



SD Acquisition, Inc.
d.b.a. CETAC Technologies
14306 Industrial Road
Omaha, Nebraska 68144, USA
Phone (402) 733-2829
Fax (402) 733-5292
e-mail: custserv@cetac.com




620056 September, 2001

Tefzel and Teflon are registered trademarks of E.I. Dupont de Nemours



ASX-100 Rotary Trays & Sample Racks


PART #

| | | |
|---|--|---|
|  | <p>Rotary tray with 15 positions (for all instruments except Perkin Elmer ELAN 5000 ICP-MS)</p> | <p>SP5464</p> |
|  | <p>Rotary tray with 10 positions (for Perkin Elmer ELAN 5000 ICP-MS instruments only)</p> | <p>SP5465</p> |
|  | <p>24 position rack, 11.5 mm diameter hole, with cover</p> <p>24 position rack, 14.0 mm diameter hole, with cover</p> <p>24 position rack, 15.0 mm diameter hole, with cover</p> <p>48 position rack, 8.0 mm diameter hole, with cover</p> <p>96 position rack, 8.0 mm diameter hole, with cover</p> <p>96 position rack, 1 mL volume hole, with cover (no vials, samples deposited directly in holes)</p> | <p>SP5404</p> <p>SP5405</p> <p>SP5463</p> <p>SP5406</p> <p>SP5407</p> <p>SP5462</p> |




PART #

| | |
|---|--|
|  | Vial kit (Teflon [®] PFA) for 15 position rotary tray SP5537 |
|  | Vial kit (Teflon [®] PFA) for 10 position rotary tray SP5543 |

For use with 24 position rack, 11.5 mm holes (SP5404)





| | |
|---|---|
|  | 0.5 mL Teflon [®] PFA vial with cap, 11.5 mm diameter hole (24 each) SP5473 0.2 mL polypropylene screw cap vial, 11.5 mm diameter hole (1000 each) SP5474 |
|---|---|

PART #

| | |
|---|--|
|  | <p>0.3 mL polypropylene screw cap vial, 11.5 mm diameter rack hole (1000 each) SP5475</p> |
|  | <p>Screw cap for 0.3 mL or 0.5 mL polypropylene vials (1000 each) SP5538</p> |
|  | <p>Teflon[®]-lined insert for screw cap (1000 each) SP5539</p> |

For use with 24 position rack with 14.0 mm diameter holes (SP5405)





PART #

| | | |
|---|---|---------------------------|
|  | <p>1.5 mL Teflon[®] PFA vial, 14.0 mm diameter (24 each)</p> | <p>SP5472</p> |
|  | <p>1.5 mL polypropylene conical vial, 14.0 mm diameter (1000 each) 1.5 mL polypropylene conical vial, 14.0 mm diameter (100 each)</p> | <p>SP5540 SP5540A</p> |
|  | <p>Cap for 1.5 mL polypropylene conical vial (1000 each) Cap for 1.5 mL polypropylene conical vial (100 each)</p> | <p>SP5541 SP5541A</p> |
|  | <p>4.0 mL Teflon[®] PFA vial, 15.0 mm diameter (24 each)</p> | <p>SP5482</p> |

PART #



| | | |
|--|--|--------|
|  | Cap for 4.0 mL Teflon® PFA vial (24 each) | SP5556 |
|  | 20mL Teflon® PFA vial (10 each) | SP5804 |
|  | Cap for 20 mL Teflon® PFA vial (10 each) | SP6008 |

For use with 48 position rack with 8.0 mm diameter holes (SP5406)

| | | PART # |
|---|--|---------------|
|  | 0.5 mL Teflon® PFA vial with cap, 8.0 mm diameter (48 each) | SP5477 |
|  | 0.5 mL polypropylene snap-cap vial, 8.0 mm diameter (1000 each) | SP5478 |
|  | 0.5 mL polypropylene screw cap vial, 8.0 mm diameter (1000 each) | SP5479 |
|  | Screw cap for 0.5 mL polypropylene vials, 8.0 mm diameter (1000 each) | SP5511 |

For use with 96 position rack with 8.0 mm diameter holes (SP5407)

PART #

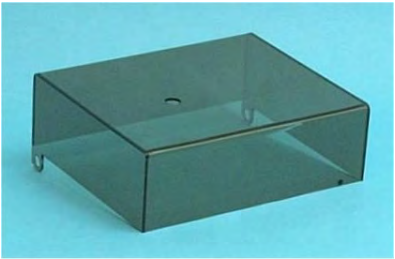
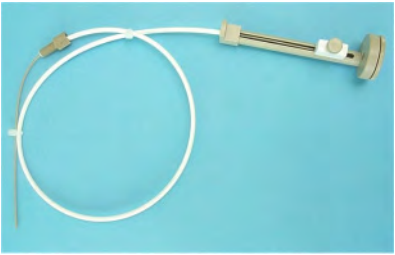

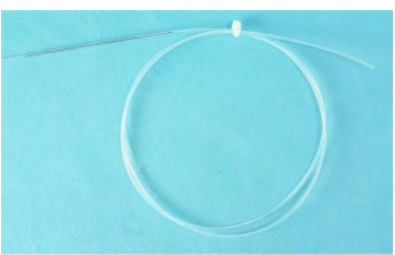
| | |
|---|---|
|  | <p>1.0 mL polypropylene vial, 8.0 mm diameter holes (1000 each)</p> <p>SP5480</p> |
|  | <p>Plug cap for 1.0 mL polypropylene vials (960 each)</p> <p>SP5542</p> |

ASX-100 Spare Parts

| | | PART # |
|---|----------------------------------|---------------|
|  | 24 volt power supply | SP5526 |
|  | Serial cable | SP5341 |
|  | Z-Axis rotor disc assembly | SP5960 |
|  | Z-Axis rotor clamp and screw kit | SP5964 |

ASX-100 Spare Parts

PART #

| | | |
|---|--|--------|
|  | Cover with magnet | SP5525 |
|  | Z-Axis drive assembly | SP5522 |
|  | Sample probe, Tefzel [®] | SP5444 |
|  | Sample probe, Teflon [®] encapsulated | SP5616 |